

Installation Guide


**PTA-60HD Patient Engagement Long Arms with GCX Channel Interface
75mm X 75mm Extended VESA, Heavy Duty**



Refer to the label on the Pivot Block to ensure that the total weight of the device and enclosure (if applicable) does not exceed the weight rating of the arm.

PTA-60HD: 60 in [150 cm] Arm: Load Range: 6.6 - 7.7 lb / 3 - 3.5 kg



PTA-60HD: 60 in [150 cm] Arm: Load Range: 13.2 - 15.4 lb / 6 - 7 kg



**Use caution when handling, unpacking and installing the Long Arm.
Internal springs may cause the Arm to expand suddenly and unexpectedly.**

Do not use the Long Arm as a hoist lever or mobility aid.




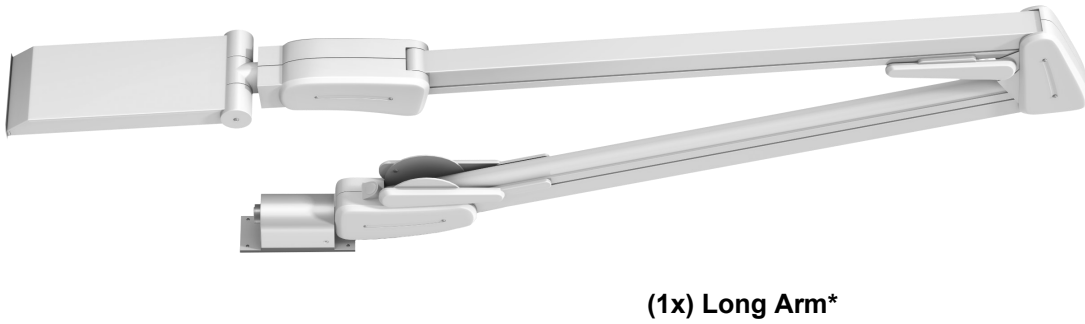

(1x) Adjustable Stop




(1x) T10



(1x) 1/8in

* The arm may come with pre-installed cable(s) - see product description for details

1

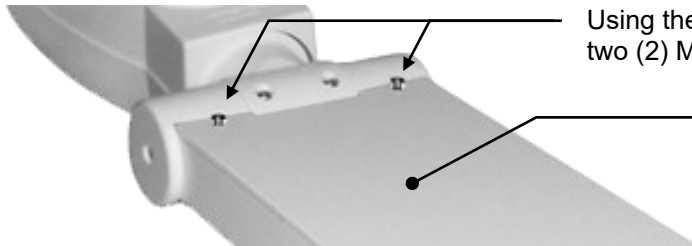


Using the supplied T10 Torx wrench, remove two (2) M3 Flat Head Torx screws and set aside


Remove cover and set aside



Do not remove any screws from opposite side of arm.




2

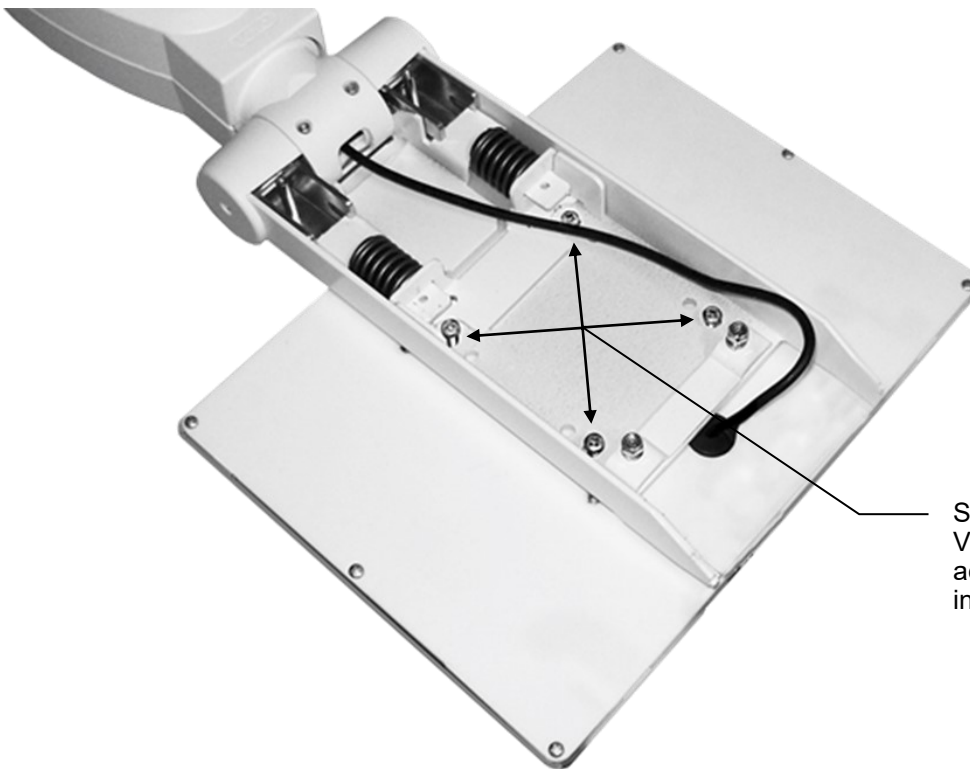


Secure device to the 75 x 75mm VESA mounting pattern in accordance with manufacturer's installation guide

3

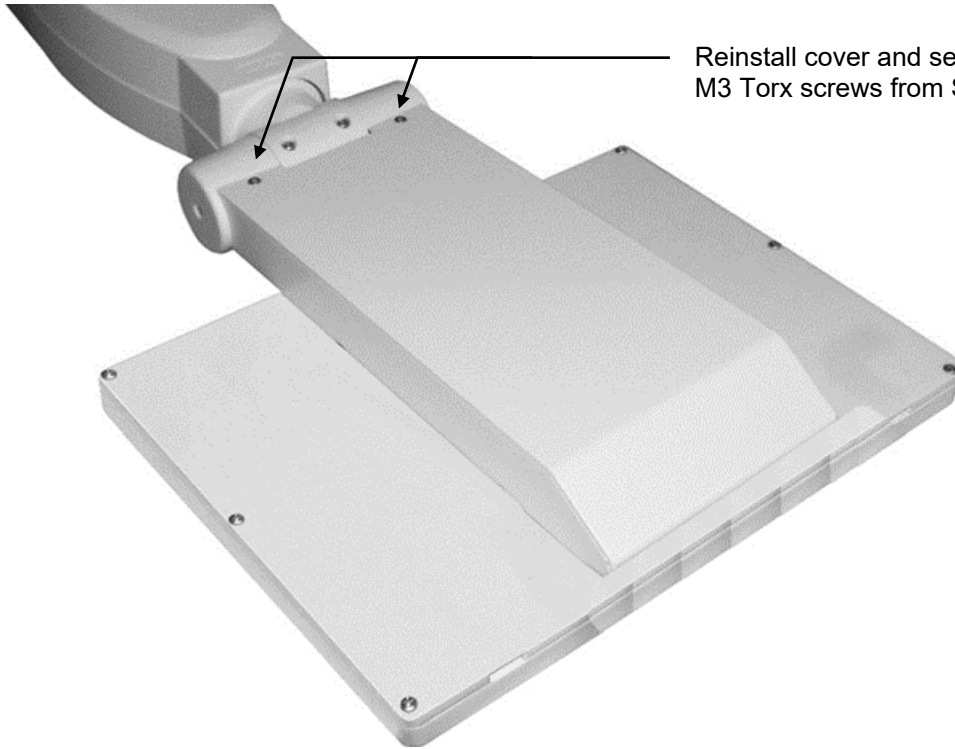

Reinstall cover and secure with the two (2) M3 Torx screws from Step 1



4



4a Guide the **adjustable stop** into the channel and secure in the desired mounting location

4b Slide the Long Arm into the top of the channel until it rests on the **adjustable stop**

With the supplied 1/8" hex wrench, turn the four (4) set screws until they engage the channel using the "ball-end" side of the hex wrench. Then, tighten the four (4) set screws using the short arm of the hex wrench



(1x) Adjustable Stop

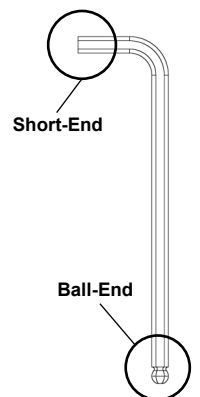

Routine Maintenance

Periodically inspect all fasteners associated with the mounting system. Tighten or adjust fasteners as necessary for optimal operation and safety.

Cleaning the Mounting Assembly

1. The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g. diluted bleach, ammonia, or alcohol solutions).
2. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone or trichloroethylene.
3. Do not use Steel wool or other abrasive material.
4. Damage caused by the use of unapproved substances or processes will not be warranted. It is recommended that you test any cleaning solution on a small area of the mounting assembly that is not visible to verify compatibility.
5. Never submerge or allow liquids to enter the mounting assembly. Wipe any cleaning agents off of the assembly immediately, using water dampened cloth. Dry the assembly thoroughly after cleaning.

CAUTION: GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted devices or accessory equipment, refer to the specific instructions delivered with those products.